


VaxAlert™ USB

SENSITECH


Instructions for Use

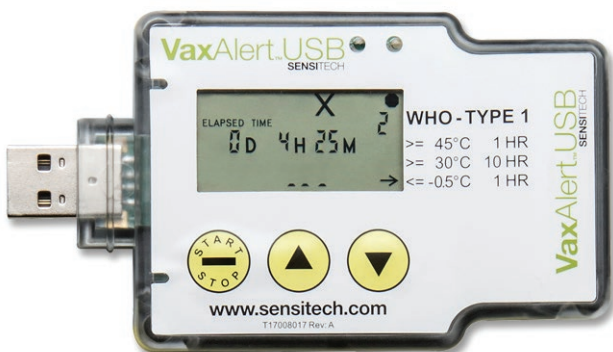

Sensitech Inc. • 800 Cummings Center, Suite 258X • Beverly, MA 01915
1-800-843-8367 • +1-978-927-7033 • Fax 978-921-2112 • www.sensitech.com


VaxAlert™ Display and Operation Features

The figure below illustrates the VaxAlert™ indicator with all screen icons simultaneously displayed, along with supporting and navigational information on the product label. This display image is not representative of the device in the use environment. (See following sections for additional information)

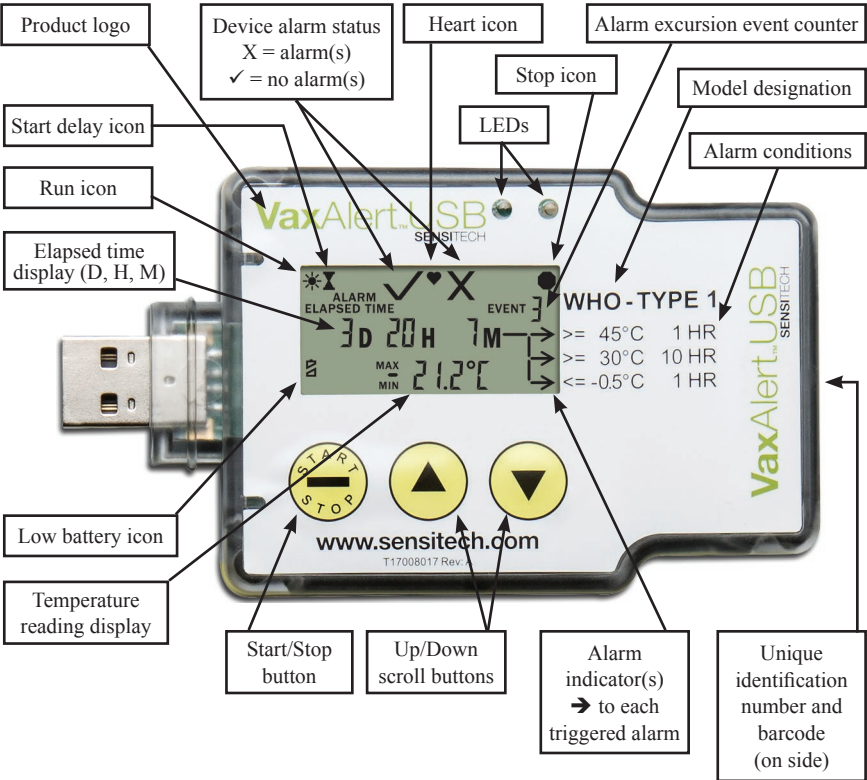


Starting the VaxAlert

1. Prior to starting the VaxAlert, the display will present a blinking heart icon (♥), to indicate the device is powered and ready to start

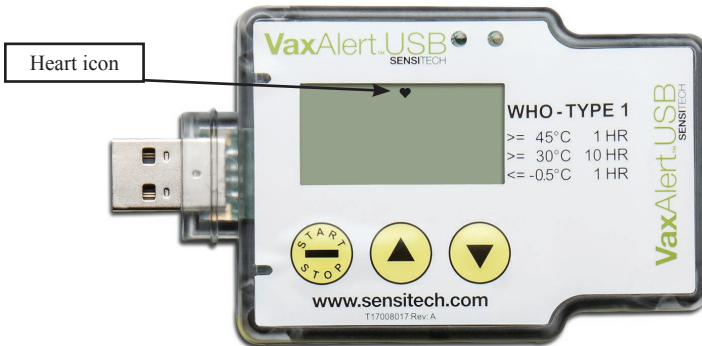


2. Press and hold the Start/Stop button for 3 seconds. The device will display the start delay screen as shown below (run icon (⌘) and start delay icon (⌚) are displayed). The display will count down the programmed start delay time until 0 minutes remain. At the end of the start delay countdown, the start delay icon will turn off and the VaxAlert will enter measurement (run) mode.

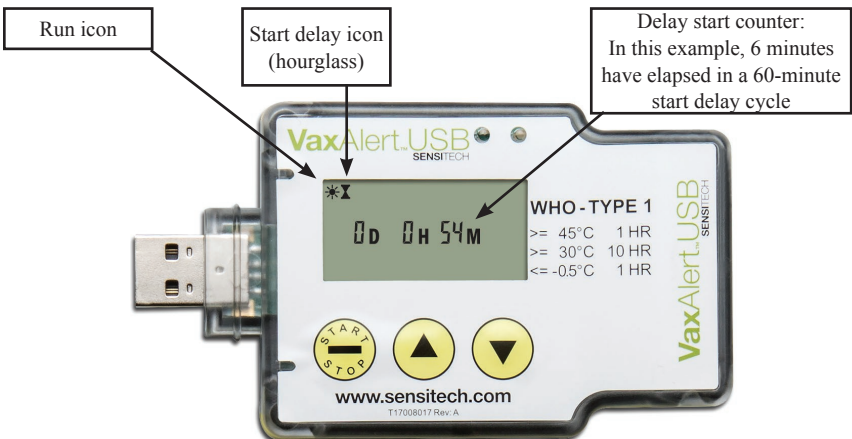


3. In measurement mode, the VaxAlert display will present elapsed trip time, last measured temperature, and alarm condition/excursion event information (if alarm activity is recorded).

VaxAlert in Measurement Mode With Alarms

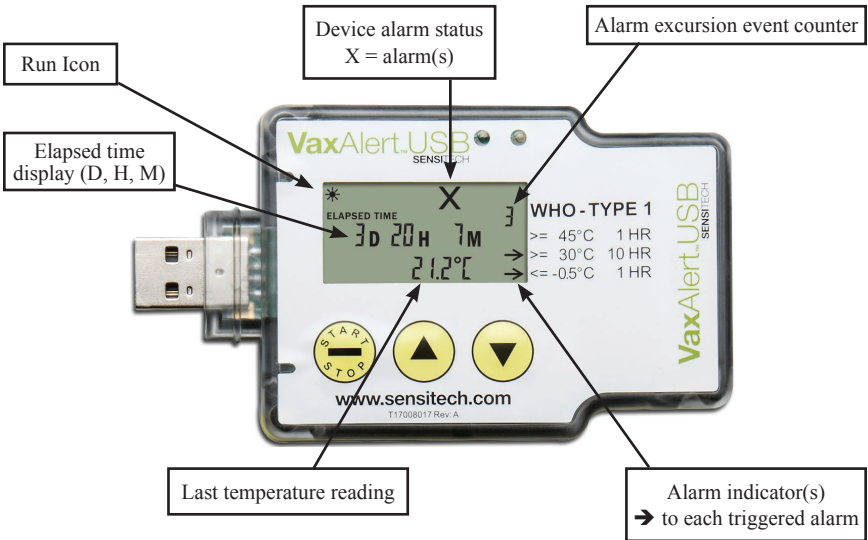


VaxAlert in Measurement Mode Without Alarms

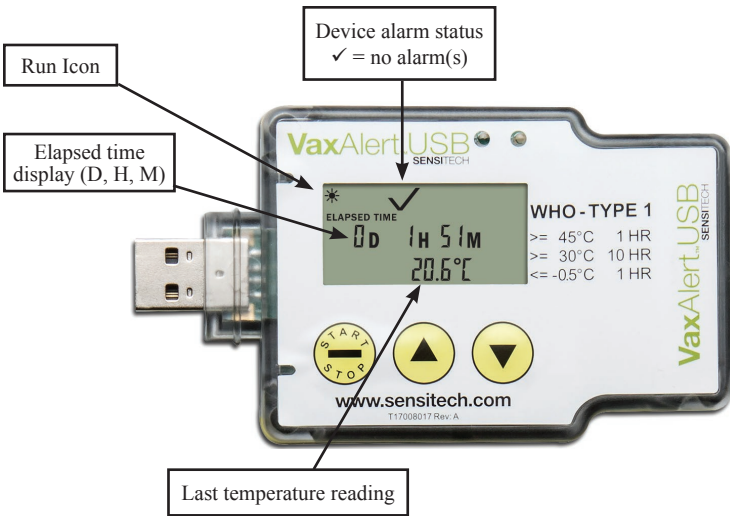


Stopping the VaxAlert

1. Press and hold the Start/Stop button for 3 seconds. The VaxAlert will display the stop mode screen as shown below (stop icon (●) is displayed).
NOTE: The VaxAlert is programmed to automatically stop after 20 days of elapsed trip time.

VaxAlert in Stop Mode With Alarms

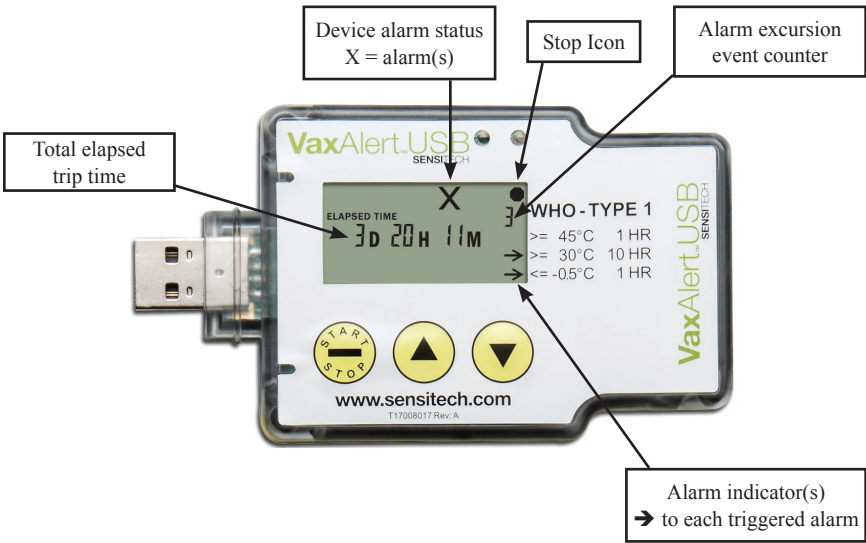


VaxAlert in Stop Mode With Alarms

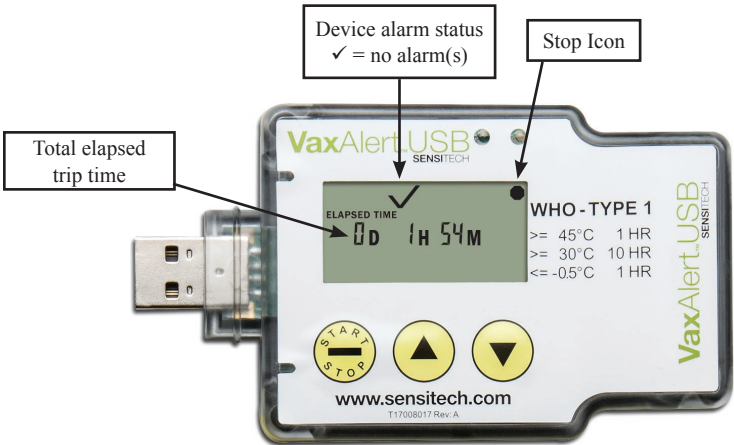

Retrieving alarm event information from the VaxAlert (HISTORY mode):


1. If the VaxAlert experiences alarm events (excursions), the device will record detailed information for up to nine total alarm events (three for each of the alarm settings). The alarm history information will be retained in the VaxAlert and can be viewed for a minimum of six months after stopping the device.
2. To view the alarm event history, press the ▲ or ▼ scroll buttons (in stop or measurement mode). The VaxAlert will display a history mode screen as shown below. Repeated presses of the ▲ or ▼ scroll buttons will cycle the alarm event history screens through all recorded alarm events (up to 9 maximum events).
3. During history mode operation, the screen will return to the stop or measurement mode screen if no additional button presses are initiated within 15 seconds. If the VaxAlert has not recorded any alarms, activating the ▲ or ▼ scroll buttons will not impact the display.

VaxAlert In History Mode, High Alarm Event

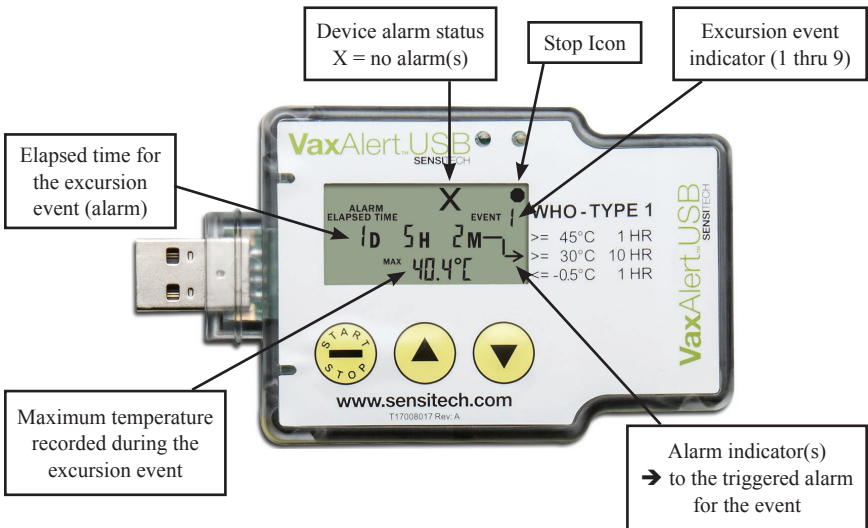


Note: In the example above, the first alarm event for this trip is a $\geq 30^{\circ}\text{C}$, 10 HR alarm at 1 day, 5 hr and 2 minute elapsed time. The maximum temperature recorded during the $\geq 30^{\circ}\text{C}$ 10 HR alarm event is 40.4°C .

VaxAlert In History Mode, Low Alarm Event

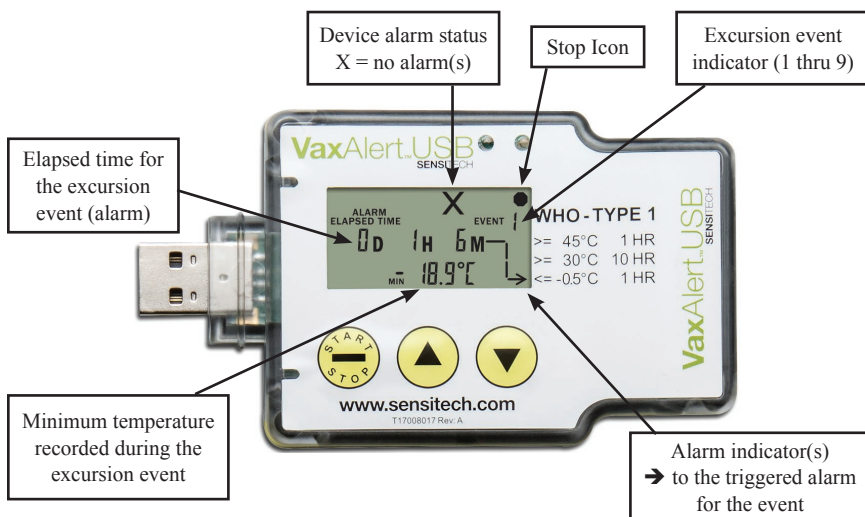

Note: In the example above, the first alarm event for this trip is a $\leq -0.5^{\circ}\text{C}$, 1 HR alarm at 0 day, 1 hr and 6 minute elapsed time. The minimum temperature recorded during the $\leq -0.5^{\circ}\text{C}$ 1 HR alarm event is -18.9°C .

VaxAlert In History Mode, High Alarm Event

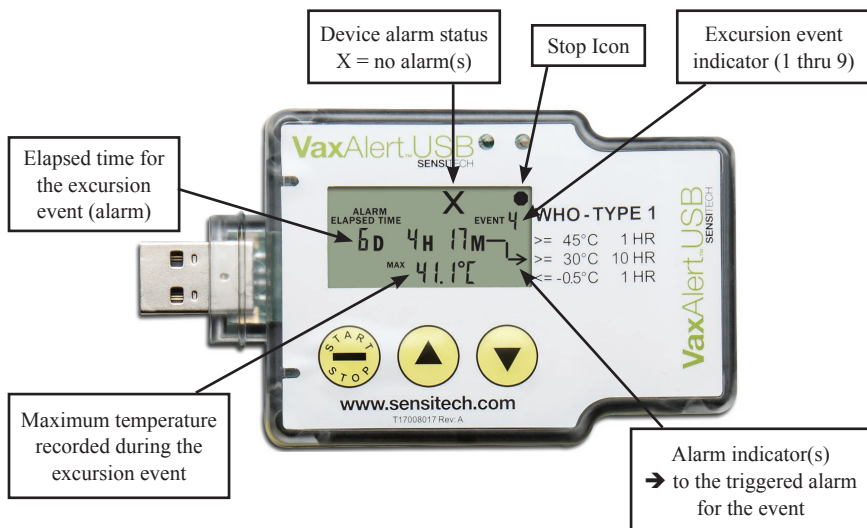

Note: In the example above, the fourth alarm event for this trip is a $\geq 30^{\circ}\text{C}$, 10 HR alarm at 6 day, 4 hr and 17 min elapsed time. The maximum temperature recorded during the $\geq 30^{\circ}\text{C}$ 10 HR alarm event is 41.1°C .

Accessing the VaxAlert USB PDF Report

1. On arrival, remove VaxAlert USB from the shipping container immediately.
2. To stop monitor, press and hold stop button for 3 seconds and verify the “stop” icon (●) on LCD.
3. Remove the protective cap and plug VaxAlert USB into USB port on PC.
4. After blinking LEDs light to solid green, double-click the PDF icon to view PDF report.

Battery Notes

The VaxAlert contains a CR Lithium battery. Please observe the following safety precautions.

- a. Dispose of or recycle the battery in accordance with your local regulations.
- b. Do not expose the device to extreme temperatures as this may lead to the destruction of the battery and could cause injury.
- c. Keep out of the reach of children.
- d. Battery status is indicated on the screen at the bottom left corner. Accuracy and proper function of the device cannot be assured once the low battery signal icon is displayed.

For more information, contact our client services group at 800-843-8367.

