


# TempTale® Ultra BLE


## Getting Started Guide

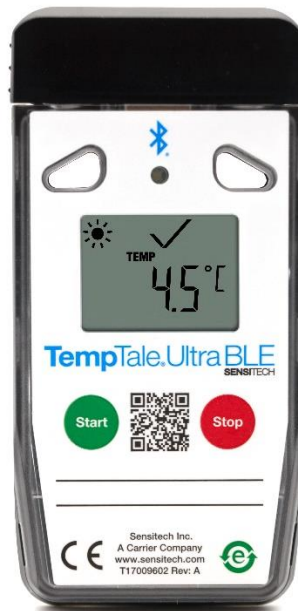


For a full-size printout of this Guide, go here: <https://www.sensitech.com/en/support/user-manuals/>  
**Minimum System Requirements • iPhone 7 or higher** running iOS 11 or higher • **Android 7.1+** • **Samsung Galaxy 8**  
**Technical Support** [sensitech.support@carrier.com](mailto:sensitech.support@carrier.com) or Sensitech EMEA: +31 (0)252 211 108

1. On the smartphone, from the Apple Store or Google Play store, download and install the TempTale® App (see *figure 5*).
2. Open the TempTale® App; allow the app access to the smartphone Bluetooth (tap OK).


**3. – Tap Get Started.**

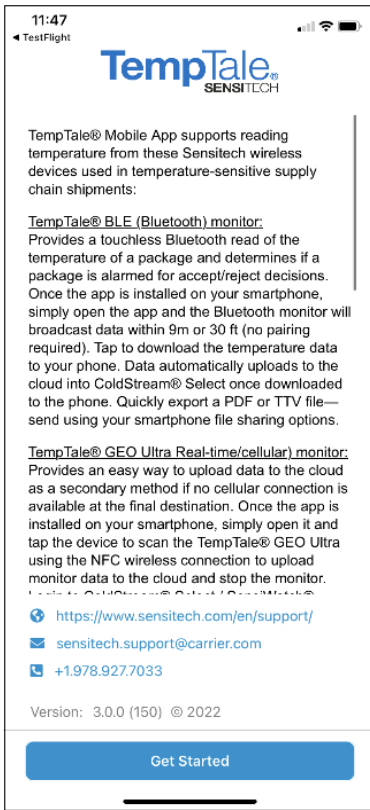

**4. – Tap both I accept options then tap I Agree.**

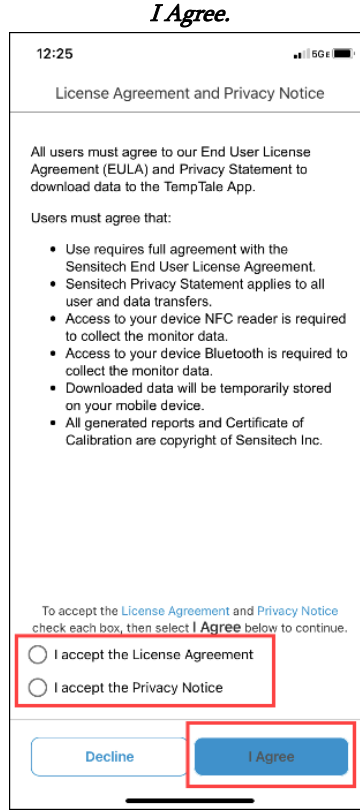

**5. – Complete and Save User Profile.**

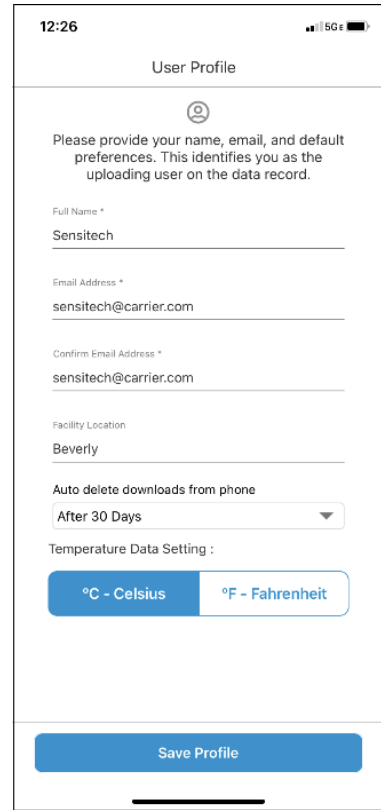


Once the TempTale® App opens, the app automatically connects to TempTale® Ultra BLE monitors within range and displays a list of monitor cards on the **Nearby BLE Monitors** tab (*figure 1*). View monitor data by downloading data to the TempTale® App.




**figure 1 – Nearby BLE Monitors tab**

**Tap white card to download monitor data to app (monitor card turns blue).**

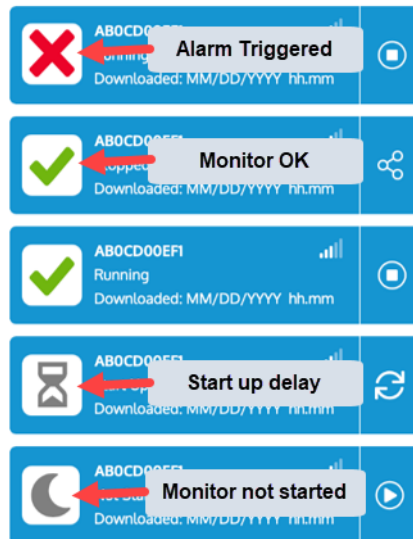

**figure 2 – Monitor card Icons**

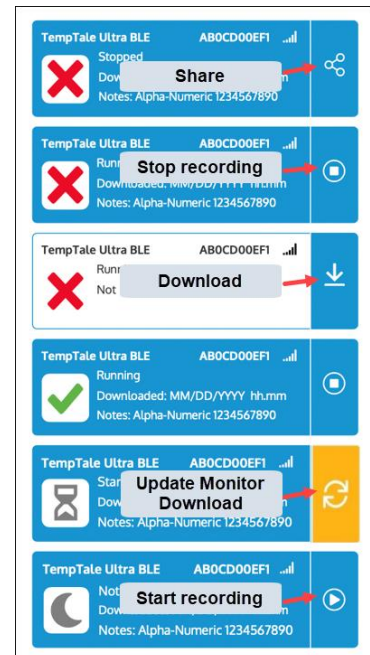

**figure 3 – Monitor card Action buttons**

**Tap a monitor card to view its details.**

**figure 4 – Monitor Card Details**

**Nearby BLE Monitors tab Toolbar icons**

	<b>Bluetooth®</b> – tap to return to the <i>Nearby BLE Monitors</i> tab
	<b>NFC Scan</b> – tap to scan NFC monitors; to download monitor data, touch phone to monitor
	<b>Download All</b> – tap to download multiple monitors' data
	<b>Action menu</b> – tap to <b>Start/Stop, Reset, Update, Export, or Delete</b> (data from app)

**Monitor card Details, Toolbar icons**

	<b>Home</b> – tap to go to <i>My Downloads</i>
	<b>Share</b> – tap to Export to PDF or TTV
	<b>Temp Graph</b> – tap to view time/temperature details
	<b>Delete Monitor Data from App</b> – clears downloaded monitor data from app
	<b>Action menu</b> – tap to <b>Start/Stop, Reset, Update, Export, or Delete</b> (data from app)

**Download the TempTale® Ultra BLE Monitor Data Using the TempTale® App.**

**Single Monitor Data Download**

On the *Nearby BLE Monitors* tab, on any white monitor card, tap **Download** (figure 7).

**Note: Once downloaded, the monitor card turns blue.**

**Multiple Monitor Data Download**

- On the *Nearby BLE Monitors* tab, on the bottom toolbar, tap **Download All**.

- Select the state that you want the monitor in after download is complete:
  - Stop Monitor:** Stop recording.
  - Stop Monitor and Reset:** Stop recording and reset with same configuration (for multi-use configured monitors only).
  - Keep Monitor Running:** Continue recording.

**Additional Actions**

- On the bottom toolbar, tap **Actions**.

- Select **Start/Stop, Reset, Update, Export, or Delete** (removes the monitor card and its data from the app).

**Export and Share the TempTale® Ultra BLE Monitor Data using the TempTale® App**

To export Monitor Data, from the Monitor Details view:

- Tap **Share**.
- On the bottom toolbar, tap **Share**.  
**Share a PDF or TTV file.**
- With **PDF** selected you can:
  - Scroll to tap the **Share** option: email, text, etc.

- Tap **Export**.

**Note: If not stopped, monitor continues recording after Export.**

**Add Originator Notes (Optional)**

Originator Notes pass information to the Delivery Driver and the Receiver (for example, shipment tracking ID).

- Tap the white card of a **Not Started** monitor.
- Tap **Edit Note**

- Enter text.
- Tap **Done**.

**Note: For multiple use, configured monitors, update Originator Notes before starting the next trip.**

**Manually Start the Monitor Recording**


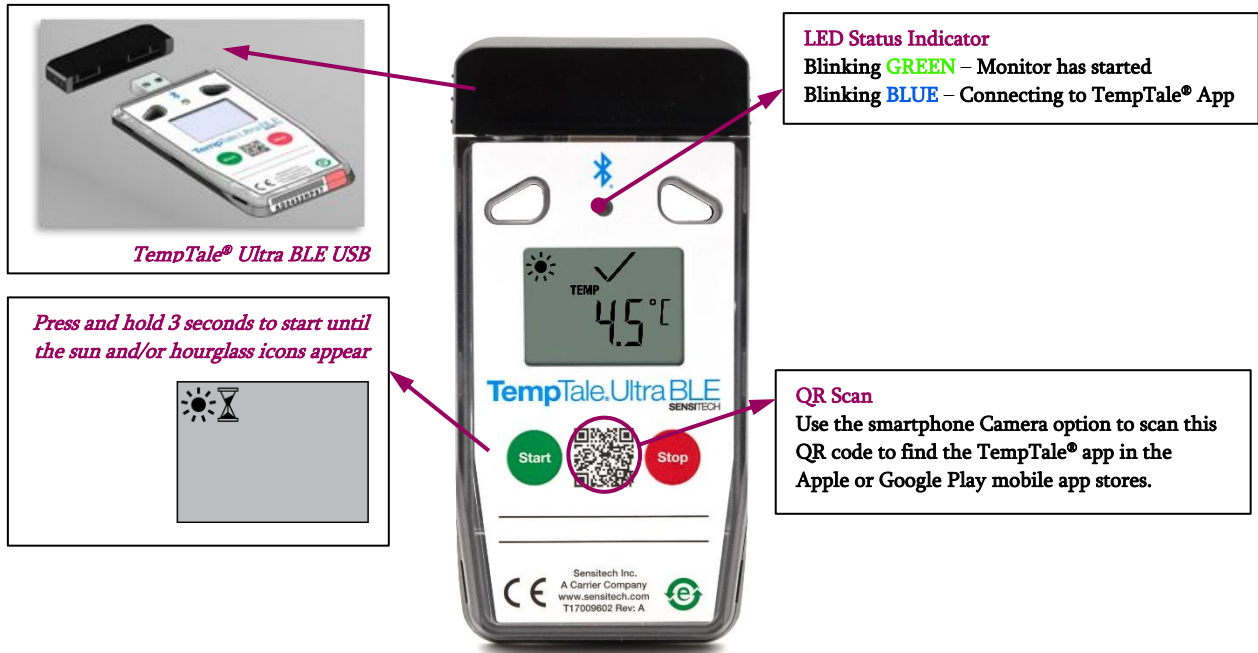


figure 5 – TempTale® Ultra BLE monitor running


**Restart/Reset the Monitor from the TempTale® App (multi-use configured monitors only)**

- If the monitor is running, tap the white area of the monitor card; from **Monitor Download Options**, select **Stop Monitor and Reset**.
- If the monitor is stopped, tap the blue area of the monitor card, and tap **Actions>Reset**.

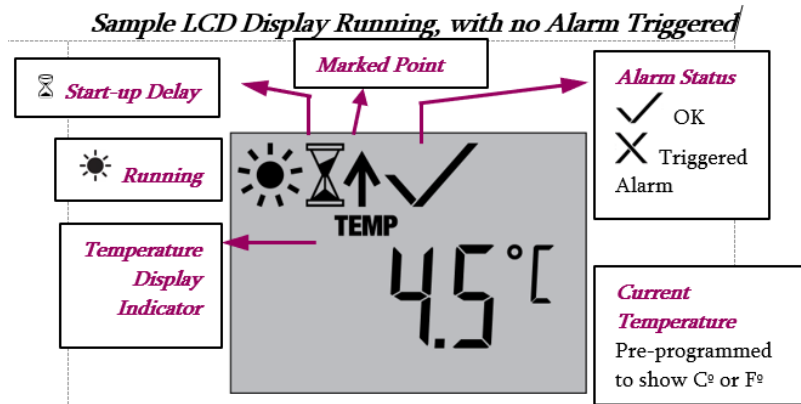

**Manually Stop the Monitor Recording**

Push and hold **Stop** until the **Stop Sign** icon displays.

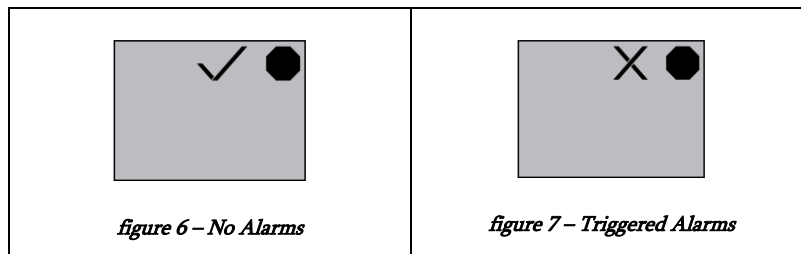

**Manually Reset the Monitor (multi-use configured monitors only)**

1. Press and hold **Stop** (8 seconds) until the blinking **CF** (figure 8) displays on the LCD, followed by **SEt** (figure 9).



2. Release the **Stop** button; the blank LCD indicates that the monitor is reset and ready for use.

Bluetooth® is a registered trademark of Bluetooth SIG.